



**Lifelines**  
neuro



# R40 and R40 24

EEG Amplifiers

MADE IN  
BRITAIN



**USER MANUAL**

Imagine EEG Anywhere



**Lifelines Ltd,**




7 Clarendon Court, Over Wallop, near Stockbridge,  
Hampshire SO20 8HU, UK  
Telephone +44 (0)1264 782226  
www.LLines.com  
sales@LLines.com



**Incereb Ltd.**

3015 Lake Drive, Citywest  
Dublin D24 DKP4, Ireland



Doc No:	51262-006
Part No:	51262-006
Issue:	2.0
CCN:	CCN126
Created	 Digitally signed by Geoff Salter Date: 2020.04.22 10:45:18 +01'00'
Checked	 Digitally signed by David Hulín DN: cn=David Hulín, o=Lifelines Ltd, ou=Development, email=david.hulin@llines.com, c=GB Date: 2020.06.15 14:25:06 +01'00'
Approved	 Digitally signed by Geoff Salter Date: 2020.06.15 14:29:38 +01'00'

### Customer Responsibility

The R40 amplifier is reliable only when operated and maintained in accordance with the instructions contained in this manual, accompanying labels, and inserts. A defective system should not be used. Parts that may be broken or missing or those that are clearly worn or contaminated should be replaced immediately with new original replacement parts that have been manufactured by or are available from Lifelines Neuro.

The owner of this system has the sole responsibility for any malfunction resulting from improper use or maintenance, or repair done by anyone other than a qualified Lifelines Neuro representative and for any malfunctions caused by any parts that have been damaged or modified by anyone other than a qualified Lifelines Neuro representative.

The owner of this system has the sole responsibility for the connection of this product to other systems not satisfying the electrical safety requirements class I, type BF, standards IEC 60601-1, IEC 60601-2-26, IEC 60601-1-2 for medical devices.

## Disclaimers & Warranties

The information in this section is subject to change without notice.

Except as stated below, Lifelines makes no warranty of any kind with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Lifelines shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance or use of this material.

Lifelines shall warrant its products against all defects in material and workmanship for one year from the date of delivery.

Misuse, accident, modification, unsuitable physical or operating environment, improper maintenance or damage caused by a product for which Lifelines is not responsible will void the warranty.

Lifelines do not warrant uninterrupted or error-free operation of its products.

Lifelines or its authorised agents will repair or replace any products that prove to be defective during the warranty period, provided that these products are used as prescribed in the operating instructions in the user's and service manuals.

No other party is authorised to make any warranty to assume liability for Lifelines products. Lifelines will not recognise any other warranty, either implied or in writing. In addition, services performed by someone other than Lifelines or its authorised agents or any technical modification or changes of products without Lifelines prior, written consent may be cause for voiding this warranty.

Defective products or parts must be returned to Lifelines or its authorised agents, along with an explanation of the failure. Shipping costs must be prepaid.

Lifelines manufactures hardware and software to be used on or with standard PC-compatible computers and operating software. Lifelines, however, assumes no responsibility for the use or reliability of its software or hardware with equipment that is not furnished by third-party manufacturers accepted by Lifelines at the date of purchase.

All warranties for third-party products used within the R40 system are the responsibility of the relevant manufacturer. Please refer to the relevant documentation on each product for further details.

This document contains proprietary information that is protected by copyright. All rights are reserved. No part of this document may be photocopied, reproduced in any other form or translated into another language without the prior written consent of Lifelines.

### Trademarks

Microsoft, Windows and Windows NT are registered trademarks of the Microsoft Corporation. All other trademarks and product names are the property of their relevant owners.

### Responsibility of manufacturer

The manufacturer and distributor consider themselves responsible for the equipment's safety, reliability and performance only if:

- any peripheral equipment to be used with the R40 system is supplied by third-party providers recommended by the manufacturer;
- assembly operations, extensions, readjustments, modifications, or repairs are carried out by person authorised by the manufacturer;
- the electrical installation of the relevant room complies with the appropriate requirements;
- the equipment is used by a healthcare professional and in accordance with the instructions for use.

**NOTE:** the manufacturer has a policy of continual product improvement; hence the equipment specifications are subject to change without notice.

Check with Lifelines or your distributor if a software update is available.

**NOTE:** Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in the Appendix.

### Software and Virus Protection

Lifelines takes all reasonable steps to ensure that its software is virus-free. In line with modern computing practice, it is advisable that continual protection against viruses, Trojans, malware, adware etc. is provided on the PC used for installation and the surrounding systems. Please note the following recommendations which should be supported by your internal IT/Computing department procedures and practices:

1. Virus protection software should be installed on every computer at risk of infection. This software should have a resident (online) shield and provide email scanning if appropriate.
2. Virus scanning should be set to manual mode or automatic if desired but at a time when the system is not being used.
3. All programs offering auto-update features, including Windows, should be set to manual or automatic if desired but at a time when the system is not being used.
4. Adopt formal departmental or organisational procedures to ensure the integrity and safe operation of the medical equipment and supporting systems.

# Contents

<b>Disclaimers &amp; Warranties</b> .....	<b>2</b>
<b>1 Overview and Technical Description</b> .....	<b>6</b>
1.1 General description.....	6
1.2 Warnings and Cautions.....	7
1.3 Explanation of symbols .....	9
1.4 The Amplifier and its parts .....	10
1.5 Specifications and safety.....	11
1.6 Description of the components .....	12
1.7 Replaceable parts.....	14
<b>2 Installation and Maintenance</b> .....	<b>15</b>
2.1 Checks for completeness and integrity .....	15
2.2 Environmental parameters for operation .....	15
2.3 Power supply connections .....	16
2.4 Use with other equipment .....	17
2.5 Interference .....	17
2.6 Maintenance and cleaning.....	18
2.7 Disposal of equipment.....	18
<b>3 Connections and Usage</b> .....	<b>19</b>
3.1 Overview .....	19
3.2 Connecting the R40 Amplifier .....	20
3.3 Starting the system .....	21
3.4 Shutdown of the system.....	21
<b>4 Trackit Software - overview</b> .....	<b>22</b>
<b>Version History</b> .....	<b>39</b>

## Appendices

Appendix 1: R40 Amplifier Specifications .....	23
Appendix 2: Additional Events Information .....	26
Appendix 3: Wireless .....	27
Appendix 4: Troubleshooting Guide .....	34
Appendix 5: Manufacturer’s Declaration .....	35

## Illustrations

Figure 1: Connecting the R40 Amplifier .....	19
Figure 2 Connecting the R40 and R40(24) Amplifier (front face).....	20
Figure 3 Connecting the R40 Amplifier (top face).....	21
Figure 4: Bluetooth pairing.....	27
Figure 5: WiFi setup .....	28
Figure 6: Unsecure network error message.....	28
Figure 7: Bluetooth connection quality monitor.....	29

# 1 Overview and Technical Description

## 1.1 General description



Federal (USA) law restricts this device to sale by or on the order of a physician.

### Indications for use

The R40 EEG Amplifier is intended to be used as a front-end amplifier to acquire, store and transmit electrophysiological signals (wireless or cabled).

### General description

The R40 EEG Amplifier is a multi-channel electroencephalograph designed for use in routine EEG and lab monitoring applications.

It is a compact USB 40-channel amplifier which incorporates 32 referential channels and 8 polygraphic channels with built-in calibration and electrode impedance measurement. A Nonin XPOD interface is provided, a Patient Event input, 2 Aux DC inputs and an Electrocap connector. Optional wireless communication is available (Bluetooth and WLAN WiFi).

Also available is the R40 (24) EEG Amplifier, which is a reduced channel variant of the R40 amplifier. The R40 (24) provides 24 referential channels and 4 polygraphic channels. In all other respects the R40 (24) amplifier is identical to the R40.

The Amplifier is intended to be connected to a PC which is powered from a medically approved power supply.

This equipment is intended only as an adjunct device in patient assessment; it must be used in conjunction with other methods of patient diagnosis. The equipment does not sustain or support life.

**NOTE:** Unless otherwise specified, throughout this manual the term "R40" refers to both the R40 EEG Amplifier and R40 (24) EEG Amplifier








### Intended User

The intended user of the equipment is a healthcare professional who has the training and knowledge to undertake EEG examinations and is familiar with EEG equipment and practice.



















## 1.2 Warnings and Cautions

	<p><b>Warning</b> sign indicates a situation or procedures that may be dangerous for the patient and/or user.</p>		<p><b>Caution</b> sign indicates a situation or procedures that may cause equipment damage or its improper usage.</p>
	<p>Do not use the R40 EEG Amplifier in an MRI environment, in an explosive atmosphere or during defibrillation.</p>		
	<p>This equipment is intended to be used by a healthcare professional and in accordance with these instructions for use which must be read in their entirety before the device is used.</p>		
	<p>This equipment is intended only as an adjunct device in patient assessment; it must be used in conjunction with other methods of patient diagnosis. This equipment is not be used for the determination of brain death.</p>		
	<p>Lifelines does not supply EEG electrodes. The unit accepts standard 1.5 mm touchproof electrodes using DIN 42802-style connectors. To ensure patient safety, the electrodes used must be approved to the Medical Device Directive 93/42/EEC in Europe or FDA cleared for use in USA.</p>		
	<p>The conductive part of electrodes and their connectors, including the Neutral electrode, should not contact other conductive parts including earth.</p>		
	<p>Lifelines does not supply the Nonin sensor. Only use the 'PureLight' sensors specified by Nonin to be used with their Oximeters.</p>		
	<p>The function or safety of the equipment could be impaired if it has been subjected to unfavourable conditions in storage or in transit. If at any time function or safety is thought to be impaired, the instrument should be taken out of operation and secured against unintended use.</p>		
	<p>Do not open or modify the equipment without the authorization of the manufacturer.</p>		
	<p>Do not touch simultaneously any accessible USB or other contacts on the PC and the patient.</p>		
	<p>Only use the PC and the medical-grade power supply as supplied or authorised by Lifelines.</p>		
	<p>Do not plug the USB connector into any device other than the PC supplied or authorised by Lifelines.</p>		
	<p>The conductive part of connectors and transducers should not contact other conductive parts including earth. Always ensure that the transducer fitted is suitable for a connection of Type BF isolation.</p>		

	Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in the Appendix.
	Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the R40 EEG Amplifier, including cables specified by Lifelines Ltd. Otherwise, degradation of the performance of this equipment could result.
	When in close proximity to the R40 EEG Amplifier, do not use mobile phones, transmitters, power transformers, motors, or other equipment that generates magnetic fields. Refer to the Appendix for more information.
	Only use approved sensors as specified by Lifelines.
	The Amplifier must only be used with the USB cable provided with the unit.
	Do not allow any liquid to enter the case of the instrument or connector. Do not use acetone on any of the instruments.
	Federal (USA) law restricts this device to sale by or on the order of a physician.








CONTRAINDICATIONS: There are no known contraindications to the use of this equipment.

### 1.3 Explanation of symbols

Symbol	Meaning	Symbol	Meaning
	Type BF applied part		Follow operating instructions
	Input/output connection		Input connection
	Special recycling required*		Bluetooth
	Consult warnings in User Manual		WLAN WiFi
	On/Off and patient event switch		Nonin Xpod Pulse Oximeter
	Remote event pushbutton		DC power
	Manufacturer		Electrocap
	Internal battery hazard - refer to section 1.7		European Representative

\* Special recycling required, do not dispose of in landfill. When this equipment has reached the end of its useful life, it must be disposed of in an environmentally-friendly way. Waste electrical and electronic equipment (WEEE) requires special procedures for recycling or disposal. This includes batteries, printed circuit boards, electronic components, wiring and other elements of electronic devices. Follow all of your respective local laws and regulations for the proper disposal of such equipment. Contact your local distributor for information concerning this.

#### Storage and transport symbols

Symbol	Meaning	Symbol	Meaning	Symbol	Meaning
	Temperature limits		Fragile		Keep dry
	Relative humidity limits		Atmospheric pressure limits		

## 1.4 The Amplifier and its parts

The R40 EEG Amplifier is a multi-channel electroencephalograph designed for use in routine EEG and lab monitoring applications.

Two variants of the R40 Amplifier are available.

The R40 EEG Amplifier is a compact USB 40-channel amplifier which incorporates 32 referential channels and 8 polygraphic channels with built-in calibration and electrode impedance measurement. A Nonin XPOD interface is provided, a Patient Event input, 2 Aux DC inputs and an Electrocap connector. Optional wireless communication is available (Bluetooth and WLAN WiFi).

The R40 (24) EEG Amplifier is a reduced channel variant of the R40 amplifier and incorporates 24 referential channels and 4 polygraphic channels. In all other respects the R40 (24) Amplifier is identical to the R40.

The Amplifier is intended to be connected to a specific PC and a medical grade power supply. Refer to Section 3.1 for details.



The PC or laptop must only be powered using the medical-grade mains power supply, as supplied or authorised by Lifelines.

The R40 EEG Amplifier comprises the following components:

Component	Part Number
R40 Amplifier	1326
R40 (24) Amplifier	1411
Amplifier USB Cable	1277
Xpod Pulse Oximeter Nonin	1327
Patient event switch	1353

**NOTE:** The Oximeter sensor is a consumable and is not supplied by Lifelines. Only use the 'PureLight' sensors specified by Nonin for use with their Oximeters.

## 1.5 Specifications and safety

Refer to **Appendix 1** for specifications.

The amplifier has been certified and complies with the following standards:

Standard	Description
IEC 60601-1 and IEC 60601-2-26	Standard for medical electrical equipment, general requirements and particular requirements for EEG systems.
IEC 60601-1-6	Collateral standard for usability.
ANSI/AAMI ES 60601-1	AAMI Deviations from IEC 60601-1 (USA).
CAN/CSA 22.2 No 601.1 M90	Canadian standard for medical electrical equipment, general requirements.
<b>IEC 60601-1-2</b>	<b>Standard for medical electrical equipment, EMC requirements, calling:</b>
*CISPR11	Conducted Emissions, Group 1, Class B
CISPR11	Radiated Emissions, Group 1, Class B
IEC61000-4-2	Electrostatic Discharges
IEC61000-4-3	Immunity - Radiated RF Field
*IEC61000-4-4	Immunity - Transients Bursts
*IEC61000-4-5	Immunity - Surges
IEC61000-4-6	Immunity - Conducted
IEC61000-4-8	Immunity - Power frequency fields
*IEC61000-4-11	Immunity - Voltage dips, interruptions
*IEC61000-3-2	Harmonic Emissions
*IEC61000-3-3	Voltage Fluctuations/flicker

*\*Note: Compliance is provided by the PC.*

### Classification of system

Classification	Clinical use
Degree of protection against electrical shock	Class I. Type BF applied parts
Type of protection against electrical shock	Optically isolated USB amplifier Mains isolation transformer for PC
Degree of protection against harmful ingress of water	Ordinary (no protection)
Mode of operation	Continuous
Degree of safety of application in the presence of a flammable anaesthetic mixture with air or with oxygen or nitrous oxide	Not suitable

## 1.6 Description of the components

### The R40 Amplifier



The R40 USB 40-channel amplifier incorporates 32 referential channels and 8 polygraphic channels with built-in calibration and electrode impedance measurement. A Nonin XPOD interface is provided, a Patient Event input, 2 Aux DC inputs and an Electrocap connector. The Amplifier has built in type-BF patient isolation and has a USB interface to the PC. Optional wireless communication is available (Bluetooth and WLAN WiFi).

The R40 (24) EEG Amplifier is a reduced channel variant of the R40 amplifier. The R40 (24) provides 24 referential channels and 4 polygraphic channels. In all other respects this amplifier is identical to the R40.

### Applied parts

#### EEG Electrodes

The amplifier connects to standard 1.5mm touchproof EEG recording electrodes arranged in a standard 10-20 pattern, attached to the patient's head.

	Lifelines does not supply EEG electrodes. The Amplifier accepts standard 1.5 mm touchproof electrodes using DIN 42802-style connectors. To ensure patient safety, the electrodes used must be approved to the Medical Device Directive 93/42/EEC in Europe or to the relevant local standards outside Europe.
	The conductive part of electrodes and their connectors, including the Neutral electrode, should not contact other conductive parts including earth.

### Oximeter Sensor

An optional oximeter sensor attaches to the patient's finger

### Patient Event pushbutton

The Patient Event Pushbutton is used by the patient to mark the instance of a significant event.

### Aux DC Inputs

The Auxiliary DC inputs are intended for the connection of patient-attached transducers which are passive or battery-powered such as sleep sensors. They must be insulated with no accessible conductive parts.

### USB Cable

The Amplifier plugs directly into a USB port on the PC.



The Amplifier must only be used with the USB cable provided with the unit.

### Medical grade AC/DC mains power supply module for Laptop PC

Where EEG studies are conducted within the patient environment the leakage current must be controlled. The laptop PC mains power supply must be a special medical-grade type with appropriate safety standards, supplied or authorised by Lifelines.



Only use the laptop and the medical-grade power supply as supplied or authorised by Lifelines. Do not use the standard laptop power supply

### The Setup and Recording Software

The R40/Trackit setup software runs under Microsoft Windows XP, Windows Vista, Windows 7, 8 or 10 on the host PC and is used to setup and review the R40 Amplifier and to record on to the PC.

#### Functions of the software:

- Setup the input signals.
- Setup and download the recording template.  
This includes which electrodes are used and the recording montage.
- Perform a calibration check of the Amplifier.
- Perform an Impedance check on the Amplifier.
- Perform an EEG recording.
- View on-going EEG traces.
- Review an EEG Recording.

*Refer to the Trackit Plus software manual for more details.*

## 1.7 Replaceable parts

Lifelines Ltd. will make available on request circuit diagrams, component part lists, descriptions, calibration instructions, or other information that will assist service personnel to repair those parts that are designated by Lifelines Ltd. as repairable by service personnel.

### Internal battery replacement – service personnel only

The R40 amplifier contains a replaceable lithium ion rechargeable coin cell, type LIR2450.



Battery replacement by inadequately trained personnel could result in a hazard. It must be replaced only with the correct type and it must be installed correctly with +ve uppermost.

1. Remove four screws from underside of instrument and remove bottom of case.
2. Unclip the wraparound screen to expose the battery beneath.
3. Grasp battery between thumb and forefinger and pull it from the socket.
4. Push replacement battery into the socket ensuring +ve is uppermost.
5. Re-clip the wraparound screen and reassemble the case.



#### Battery safety instructions

Do not attempt to open, puncture, disassemble or modify the battery in any way.  
Do not subject the battery to sudden shock or heat.  
Do not dispose of battery in fire.



## 2 Installation and Maintenance

The following section must be read and understood before the equipment is switched ON.



Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in the Appendix.

The function or safety of the equipment could be impaired if it has been subjected to unfavourable conditions in storage or in transit. If at any time function or safety is thought to be impaired, the instrument should be taken out of operation and secured against unintended use.

The manufacturer should be contacted (details on page ii) for assistance, if needed, in setting up, using or maintaining the equipment; or to report unexpected operation or events.

The assembly of the system and any modifications during its service life require evaluation to the requirements of IEC 60601-1.

### 2.1 Checks for completeness and integrity

1. Remove the equipment from the packaging case(s).
2. Use the parts list to check that all ordered items have been received.
3. Check for signs of damage that may have occurred during transit or storage. If any damage is found, do not use the instrument; contact your distributor.

### 2.2 Environmental parameters for operation


The operational and storage/transportation environmental conditions are as follows:

Operational:		Storage and transport:	
Temperature	+10°C to +40°C (+50°F to +104°F)	Temperature	-10°C to +50°C (14°F to +122°F)
Relative humidity	25% to 95% non-condensing	Relative humidity	10% to 95% non-condensing
Atmospheric pressure	700 hPa to 1060 hPa	Atmospheric pressure	500 hPa to 1060 hPa

## 2.3 Power supply connections

### R40 Amplifier



Power requirements	Standard USB port (5V)
Power consumption	Maximum power from USB port: 2.5W.

	The Amplifier must only be used with the USB cable provided with the unit.
---	--

### Medical grade AC mains power supply module for Laptop PC

Where EEG studies are conducted within the patient environment the leakage current must be controlled. The mains power supply must be a special medical-grade type with appropriate safety standards, as supplied or authorised by Lifelines.

Medical grade AC mains power supply module for Laptop PC	
Mains Power input:	100–240 Vac, 47–63 Hz, 1.4 A @ 115 Vac, 0.7 A @ 230 Vac.
Output:	20 Vdc, 5.25 A.

	The laptop must only be connected to the medical-grade laptop power supply supplied or authorised by Lifelines. Do not use a standard laptop power supply. Only use the laptop supplied or authorised by Lifelines.
	To avoid the risk of electric shock, this equipment must only be connected to a supply mains with protective earth.

## 2.4 Use with other equipment

### Defibrillators and HF surgical equipment

The equipment is not defibrillator proof and should not be used in situations where a defibrillator is likely to be used. The equipment should not be used with, or in the presence of, high frequency surgical equipment.

### Other patient-connected equipment

When used simultaneously with other patient-connected equipment, for example a cardiac pacemaker or other electrical stimulator, it is unlikely that a safety hazard will arise. However always consult the documentation supplied with the other patient-connected equipment to ensure that all hazards, warnings and cautions are considered before the equipment is used together.



Non-medical equipment, when used with the system, should comply with IEC/ISO safety standards relevant to that equipment. IT equipment should comply with IEC 60950.

### Leakage current

This system is designed to comply with IEC 60601-1, the international standard for medical electronic equipment, which specifies the permissible levels of leakage current. A potential hazard exists in the summation of leakage currents caused by connecting several pieces of equipment together. Because this system can be used in conjunction with standard electronic devices, the total leakage current should be tested whenever the system is modified.

There should be no electrical connections between the system equipment, which is powered via a medical grade power supply, and any other equipment powered from another mains supply.

## 2.5 Interference

The R40 will continue to operate in the presence of radio frequency magnetic fields (RF) and the effects of electrostatic discharges (ESD) and other interference, in accordance with the requirements of EN60601-1-2. However, the R40 amplifier records signals of very low amplitude, and these signals themselves are not immune to the effects of RF, ESD and low-frequency magnetic field interference. Such interference may cause signal artefacts.

The R40 may have internal radios fitted. These are approved industry-standard Bluetooth and WiFi types which present minimal risk of reciprocal interference with other equipment.

However, when the equipment is operated with or without its Bluetooth or WiFi on, other devices in the vicinity should be moved away or turned off to reduce the likelihood of interference to the equipment or by the equipment.



Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the R40, including cables specified by Lifelines Ltd. Otherwise, degradation of the performance of this equipment could result.



When in close proximity to the R40 Amplifier, do not use mobile phones, transmitters, power transformers, motors, or other equipment that generates magnetic fields. Refer to the Appendix for more information.



Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in the Appendix.

## 2.6 Maintenance and cleaning

The R40 Amplifier requires no routine testing, calibration or maintenance procedures apart from occasional cleaning and checking for wear and damage to all parts including the accessories.

### Cleaning and disinfection

All the outer surfaces of the R40 Amplifier may be cleaned using a soft cloth moistened with water and a mild detergent solution. A low-pressure airline or a vacuum cleaner can also be used.

Disinfection of the equipment can be carried out by the use of QAC-based disinfectants. Wipes are recommended in order to prevent the ingress of any liquid into the equipment. Suitable products include Mikrozyd Sensitive Wipes (Schülke & Mayr GmbH), Microbac forte (Paul Hartmann AG), Distel Wipes (Tristel Ltd.), Mikro-Kill disinfectant wipes (Medline Industries, Inc.), Sani-Cloth HB Germicidal Wipes (PD International, Inc).

For cleaning instructions for the laptop refer to the manufacturer's documentation.



Do not allow any liquid to enter the case of the instrument or connector. Do not use acetone on any of the instruments.

## 2.7 Disposal of equipment

When the device and its parts and accessories has reached the end of its operating life, it should be disposed of in accordance with local waste regulation authority that is typically within the local government office.

## 3 Connections and Usage

### 3.1 Overview

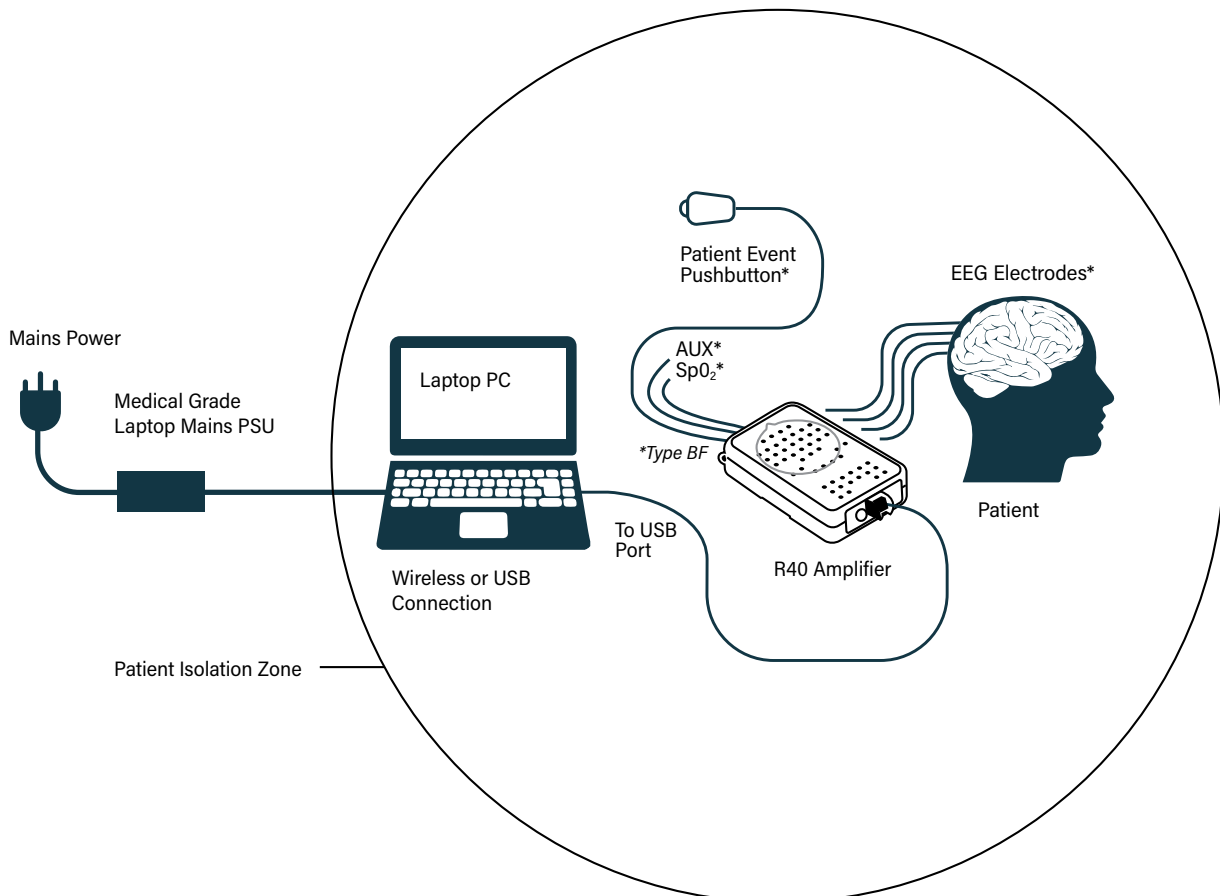


Figure 1: Connecting the R40 Amplifier

Where the entire R40 system including the PC is used within the patient environment, the mains leakage currents and safety and regulatory requirements are met by the use of the special medical-grade laptop power supply.



The laptop must only be connected to the medical-grade laptop power supply supplied or authorised by Lifelines. Do not use a standard laptop power supply.

Only use the laptop supplied or authorised by Lifelines.

### 3.2 Connecting the R40 Amplifier

The R40 Amplifier is plugged into the PC USB port using the cable supplied, part number 1277.

The USB Cable is plugged into the bottom housing of the R40 Amplifier as shown below using the RJ45 plug and into any USB port on the PC.



Figure 2 Connecting the R40 and R40(24) Amplifier (front face)

The front face of the Amplifier is laid out in a standard 10-20 format, and accommodates standard touchproof electrode leads fitted with DIN 42802 connectors.

Also on the front face of the Amplifier are the electrode impedance check set-level pushbuttons. Adjacent to each electrode is an LED indicating whether the impedance of the individual electrode is above the set-level.

	<p>The Amplifier accepts standard 1.5 mm touchproof electrodes using DIN 42802-style connectors. To ensure patient safety, the electrodes used must be approved to the Medical Device Directive 93/42/EEC in Europe or to the relevant local standards outside Europe.</p>
	<p>The conductive part of electrodes and their connectors, including the Neutral electrode, should not contact other conductive parts including earth.</p>

The top edge of the Amplifier provides for several other connections, as shown below.

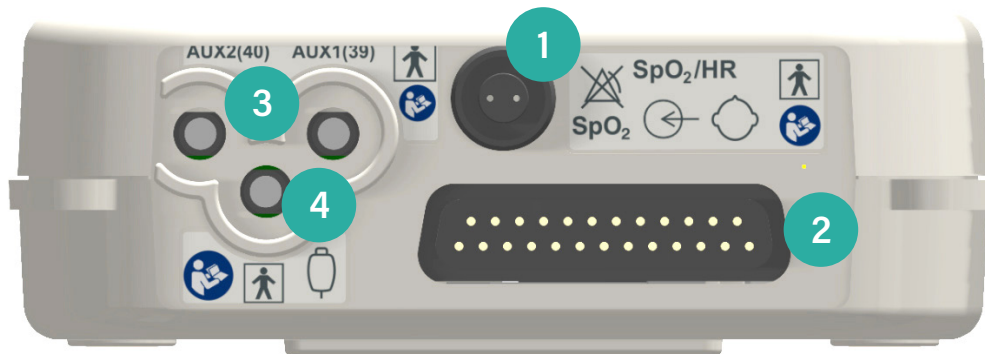


Figure 3 Connecting the R40 Amplifier (top face)

1. Nonin Xpod: the circular connector allows for the connection of a Nonin Xpod pulse oximeter for measuring SpO<sub>2</sub>.
2. Electro-Cap: the 25-way D-type connector allows for the connection of a standard Electro-Cap.
3. Aux1 and Aux2: these two 3.5mm jack connectors allow for the connection of standard transducers like Body Position, Respiration Belts etc.
4. Patient Event: this 3.5mm jack connector allows for the connection of a standard Patient Event Thumb Switch.



All these connections are Type BF isolated. The conductive part of connectors and transducers should not contact other conductive parts including earth. Always ensure that the transducer fitted is suitable for a connection of this type.

### 3.3 Starting the system

To start the system proceed as follows:

- Plug the PC into the mains supply.
- Switch on the PC and wait for Windows to load.
- Ensure R40 Amplifier is connected via the USB lead.
- Launch the Trackit Plus Software application. Refer to the Trackit Plus Software User Manual for more details.
- These procedures also apply following a mains interruption.

### 3.4 Shutdown of the system

At the completion of a study proceed as follows to shut down the system:

- Stop the recording by pressing the 'Stop Rec' button
- Exit the Trackit program.
- Shut down Windows.
- Switch off the PC and disconnect the mains supply.



## 4 Trackit Software - overview

The Trackit software is available on the included CD/USB disk or on the Lifelines FTP site. A readme file describes installation. The Trackit Software version 2.8.0.0 (or later) supports the R40 Amplifier. Check with your distributor or Lifelines if a newer version of software is available.

The Trackit software is designed to work with both the R40 Amplifier and with the optional Photic Stimulator.

The software is supported on Microsoft Windows XP, Windows Vista and Windows 7, Windows 8 and Windows 10. The USB drivers will be found on the CD. After connecting the Amplifier to the PC for the first time, at the Windows prompt, browse to the folder CD Drive:\USB Drivers. From there Windows will find the correct drivers for the version of Windows being used.

The software has the following functions:

- Define signal types: create labels to attach to inputs
- Attach the desired signal type (label) to the recording input
- Create a recording montage and download it to the amplifier
- Perform a calibration of the inputs
- Perform an impedance check on the inputs
- View ongoing signals and adjust display parameters such as chart speed and display sensitivity
- Start and stop a recording session
- Open and review EEG recordings (EDF and BDF format)

**NOTE:** See separate Trackit Plus software manual for setup and recording details.



## Appendix 1: R40 Amplifier Specifications

Lifelines reserves the right to change product specifications at any time without notice. This is in line with the company's policy of continual product development.

EEG inputs	
Number of EEG channels	R40 : 32 monopolar touchproof inputs R40 (24) : 24 monopolar touchproof inputs
ADC Resolution	24 bits
Sampling	250 - 16000 Hz
Input impedance	>20 Mohms
Common mode rejection ratio	>100dB @ 50 and 60 Hz
Equivalent input noise	<1.5 $\mu$ Vpp, <0.2 $\mu$ V rms
Gain	12 $\pm$ 0.5%
Max Input Vdiff	750mVpp (including DC)
Quantisation	0.17 $\mu$ V/bit @ Gain = 12 and Bits = 22
Bandwidth (-3dB)	DC to 4193Hz
Max common mode input voltage	0.4Vpp
Input bias current	< $\pm$ 0.3 nA
Front-end Calibration	8mVpp $\pm$ 5% at 0.98Hz
Impedance Check current	24nA $\pm$ 20% at 7.8Hz
Polygraphy inputs	
Number of polygraphy inputs	R40: 8 bipolar touchproof inputs R40 (24): 4 bipolar touchproof inputs
ADC Resolution	24 bits
Sampling	250 - 16000 Hz
Input impedance	>20 Mohms
Common mode rejection ratio	>100dB @ 50 and 60 Hz
Equivalent input noise	<1.5 $\mu$ Vpp, <0.2 $\mu$ V rms
Gain	12 $\pm$ 0.5% (AC), 4 $\pm$ 0.5% (DC)
Max Input Vdiff	750mVpp AC setting (including DC), 2.25Vpp DC setting
Bandwidth (-3dB)	DC to 4193Hz
Quantisation	0.17 $\mu$ V/bit @ Gain = 12 and Bits = 22
Max common mode input voltage	0.4Vpp
Input bias current	< $\pm$ 0.3 nA
Front-end Calibration	8mVpp $\pm$ 5% at 0.98Hz
Impedance Check current	24nA $\pm$ 20% at 7.8Hz
Aux. high-level DC Inputs	
Number of Aux channels	2 (channels 39 and 40)
ADC Resolution	24 bits
Sampling	250 - 16000 Hz
Input impedance	100 Kohms
Gain	4 $\pm$ 0.5%
Max Input Vdiff	2.25Vpp
Bandwidth (-3dB)	DC to 4193Hz max.

**Connections, ports and controls**

Electrode Input connectors	R40: 52 Touchproof 1.5mm R40 (24) 34 Touchproof 1.5mm
E-cap connector	1 Standard 25-pin D socket
Aux DC Inputs	2 Jack socket 3.5mm (Channels 39 and 40)
Patient Event Input	1 Jack socket 3.5mm
Front-panel push-buttons	1 push-button Impedance Check - 1 push-button Impedance Check +
Host PC Connector	1 RJ45 socket providing USB port (isolated from patient)
Nonin Xpod (SaO <sub>2</sub> )	1 Binder 710 series 3-pin socket
LED indicators	Impedance Check Indication (1 per channel). R40: 40 LEDs, R40 (24): 28 LEDs 5 LEDs for Impedance Check Level, 1 LED for Power On, 1 LED for Wireless operation
Micro-SD card port	1 Micro-SD socket
Internal Battery	1 type LIR2450 Lithium-ion rechargeable Coin cell
Internal beeper	

**Bluetooth Wireless**

Type	Bluetooth 4.0
Output power	11dBm max.
Output frequency	2.402 - 2.480 GHz, ISM band
Data rate	1.3 Mbps max.
Protocols	Standard Bluetooth - SPP, GATT, DUN, PAN
Modulation	GFSK, DQPSK. Frequency Hopping Spread-Spectrum (FHSS)
Error correction	Forward Error Correction (FEC), Automatic repeat request (ARQ).
Security	Authorization and authentication of devices, proprietary Interface Protocol
Type Approvals	Europe (ETSI R&TTE); US (FCC/CFR 47 part 15 unlicensed modular transmitter approval) Canada (IC RSS); Japan (MIC - formerly TELEC)
R&TTE Directive 1999/5/EC	Effective use of frequency spectrum: EN 300 328 EMC: EN 301 489-1, EN 301 489-17, EN 61000-6-2 Health and safety: EN 62479, EN 60950-1, IEC 609501
Medical Electrical Equipment	IEC 60601-1-2
Bluetooth Qualification	V4.0

**Wireless LAN**

Type	2.4 GHz IEEE Std. 802.11 b/g Wireless LAN Module
Output power	12dBm max.
Output frequency	2.412 to 2.462 GHz, ISM band
Data rate	230kbps max.
Protocols	TCP, UDP, DHCP, DNS, ICMP, ARP, HTTP Client, and FTP Client
Modulation	802.11b Compatibility: DSSS (CCK-11, CCK-5.5, DQPSK-2, DBPSK-1) 802.11g: OFDM
Error correction	Forward Error Correction (FEC)
Security	WEP-128, WPA-PSK (TKIP), WPA2-PSK (AES) proprietary Interface Protocol
FCC	Part 15.247 FCC T9J-RN171
IC	RSS-210 low-power communication device
CE	ID# 0681
REG	U9M21103-4249-C
Radio	EN 300328 V1.7.1 (10/2006)
EMC	EN 301489-1 V1.8.1 (04/2008) EN 301489-17 V2.1.1 (05/2009)
Safety	EN 60950-1:2006+A11:2010, EN 50371 2002-03

**Physical characteristics**

Weight	400g
Size	17cm x 11cm x 4cm

**Safety and EMC standards**

The system has been certified and complies with the following standards:

IEC 60601-1 and IEC 60601-2-26	International standard for medical electrical equipment, general requirements and particular requirements for EEG systems.
ANSI/AAMI ES 60601-1	AAMI Deviations from IEC 60601-1 (USA).
CAN/CSA 22.2 No 601.1 M90	Canadian standard for medical electrical equipment, general requirements.
IEC 60601-1-2	International standard for medical electrical equipment, EMC requirements, calling:
*CISPR11	Conducted Emissions, Group 1, Class B
CISPR11	Radiated Emissions, Group 1, Class B
IEC61000-4-2	Electrostatic Discharges
IEC61000-4-3	Immunity - Radiated RF Field
*IEC61000-4-4	Immunity - Transients Bursts
*IEC61000-4-5	Immunity - Surges
IEC61000-4-6	Immunity - Conducted
IEC61000-4-8	Immunity - Power frequency fields
*IEC61000-4-11	Immunity - Voltage dips, interruptions
*IEC61000-3-2	Harmonic Emissions
*IEC61000-3-3	Voltage Fluctuations/flicker

\*Note: Compliance is provided by the PC

**R40 Amplifier Classification**

Classification	Clinical use
Degree of protection against electrical shock (when connected to host system)	Type BF
Type of protection against electrical shock (when connected to host system)	Optically isolated USB amplifier Mains isolation transformer for PC
Degree of protection against harmful ingress of water	Ordinary (no protection)
Mode of operation	Continuous
Degree of safety of application in the presence of a flammable anaesthetic mixture with air or with oxygen or nitrous oxide	Not suitable

## Appendix 2: Additional Events Information

For the R40 EEG Amplifier, events types are as shown below.

- 56 Automatic events (hardware events, photic start/stop, video start/stop etc.)
- 40 user-configurable events
- Free-text events entered during acquisition

Refer to the *Trackit Plus software manual* for more information

Event List Key	Event No	Contents	Type	Size	Total size	Mapping
0	0	No event	Fixed	16x16	256	Auto
	1	Stop recording	Fixed			Auto
	2	Start recording	Fixed			Auto
	3	Door Open	Fixed			Auto
	4	Door Closed	Fixed			Auto
	5	Host On	Fixed			Auto
	6	Host Off	Fixed			Auto
	7	Low Battery	Fixed			Auto
	8	OK Battery	Fixed			Auto
	9	Imp. Check Mode	Fixed			Auto
	10	Calibrate Mode	Fixed			Auto
	11	Normal Mode	Fixed			Auto
	12	Electrodes On	Fixed			Auto
	13	Electrodes Off	Fixed			Auto
	14	Patient Event	Fixed			Auto
15	External Event	Fixed	Auto			
1	16	Awake #	User-config	16x16	256	F1
	17	Asleep #	User-config			F2
	18	Eyes open #	User-config			F3
	19	Eyes closed #	User-config			F4
	20	Lights on #	User-config			F5
	21	Lights off #	User-config			F6
	22	Drowsy #	User-config			F7
	23	#	User-config			F8
	24	Photic start	Fixed			Auto
	25	Photic stop	Fixed			Auto
	26	HV start	Fixed			Auto
	27	HV >>	Fixed			Auto
	28	HV stop	Fixed			Auto
	29	Post HV start	Fixed			Auto
	30	Post HV >>	Fixed			Auto
31	Post HV stop	Fixed	Auto			
2	32	Video start	Fixed	32x32	1024	Auto
	33	Video stop				Auto
	34	Video movement				Auto
	35	Trackit connect				Auto
	36	Trackit disconnect				Auto
	37-63	Reserved				Auto
3	64-95	?	User-config	32x32	1024	Shift F1-8 Ctrl+Shift F1-8
4	96-159	?	User-config (free text)	64x64	4096	F12

## Appendix 3: Wireless

### Introduction

The R40 Amplifier has optional built-in Bluetooth and WiFi capabilities.

Using the internal Bluetooth module in the R40, wireless connections can be established with it from a Bluetooth-enabled PC. Using the internal WiFi module in the R40 wireless connections can be established with it via a Wireless Access Point (WAP). This allows the R40 to be monitored remotely over a secure wireless link up to a range of about 100m or greater (dependent on hardware and environmental factors).

### System overview

The Bluetooth module is Bluetooth Qualified v4.0. The WiFi module is IEEE 802.11 b/g certified. For full specifications, refer below.

Bluetooth is a device to computer wireless connection and will connect to any suitably certified Bluetooth host, like a PC or laptop. The connection process uses authentication and password protection.

The WiFi (wireless LAN Module) is a device to network wireless connection and will connect to a designated network via a Wireless Access Point (WAP). The connection process uses authentication and password protection.

### Connection and use

Both the Bluetooth and WiFi connections require secure passwords to be entered.

During the Bluetooth pairing process, the correct password must be entered to establish the connection. As shown below, a secure password authorization and authentication process takes place during the pairing procedure.

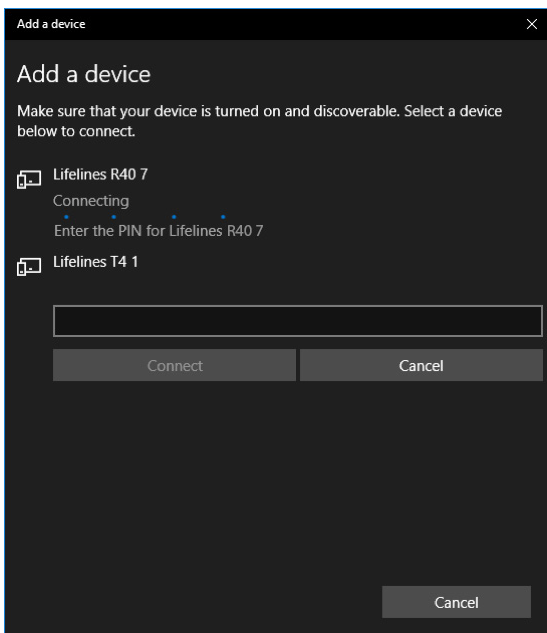


Figure 4: Bluetooth pairing

Once established, the R40 acts as the server and provides the SPP service to the PC acting as a client.

During the setup of the WiFi module, the WAP SSID is entered together with its password, as shown below.

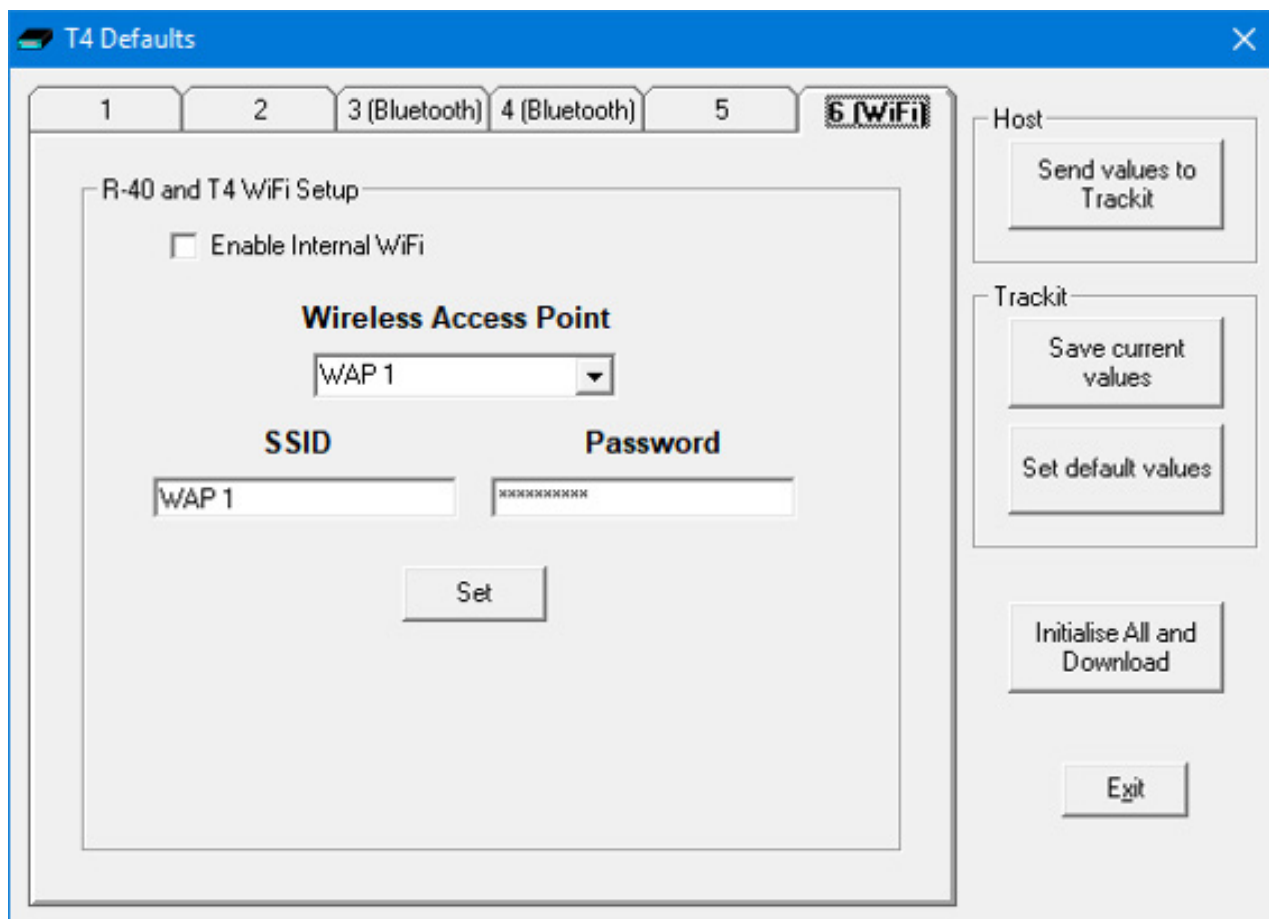


Figure 5: WiFi setup

If an attempt is made to connect to an unsecure network without a password, this is prevented and an error displayed as shown below. For maximum security it is recommended that only WPA2 access is allowed.



Figure 6: Unsecure network error message

When the Trackit application has established the Bluetooth connection, a connection quality monitor labelled “Comms.Q” is displayed in the status bar at the bottom left of the main screen, as shown below.

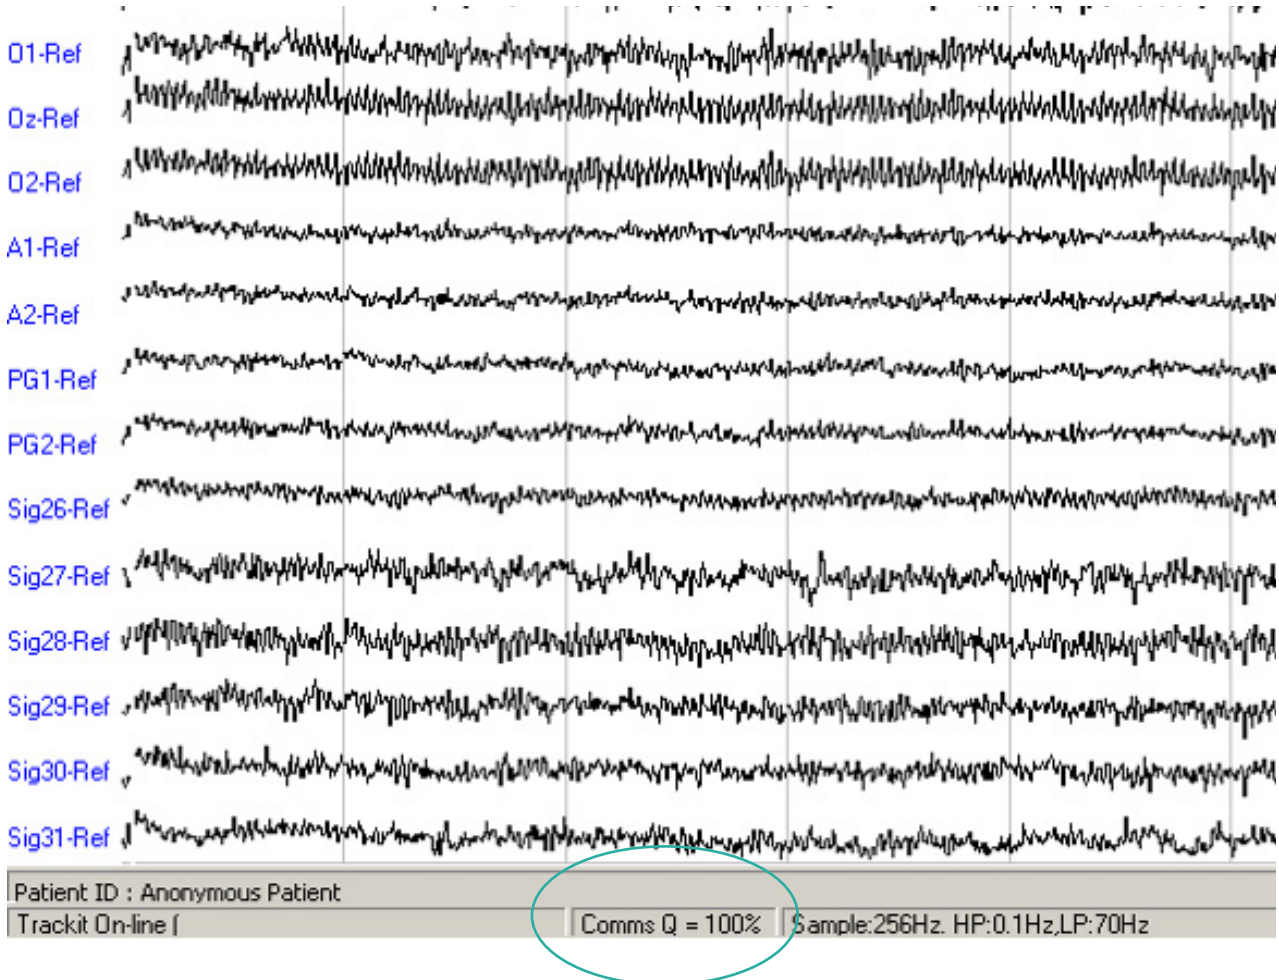


Figure 7: Bluetooth connection quality monitor.

This number given as a percentage is an approximate indication of the amount of data received as a ratio to that expected, calculated every second. It is most likely to drop below 100% when either device is at the limit of the transmission range or when either antenna is adversely obscured or under the influence of interference. It will be noticed that the wireless transmission will use its available bandwidth to try to “catch-up” after a drop in signal quality and the indication can read more than 100% momentarily. A reading, therefore, of less than 100% does not necessarily mean a permanent bad connection since data flow can increase shortly afterwards. A sustained low value over several seconds will cause the Trackit application to close the connection. If the Autoconnect feature has been enabled in Options, the application will automatically attempt to reconnect to the R40 every 10 seconds.

## Wireless Communication (general information)

### **A wireless link can be subject to interference and disruption to communication.**

Bluetooth is a wireless technology designed for short-range wireless connections between devices in a wireless personal area network (WPAN). Bluetooth is compliant with the IEEE 802.15 standard and operates in the 2.4 GHz band. WiFi is a wireless technology designed to connect devices and an infrastructure in a wireless local area network (WLAN). WiFi is compliant with various IEEE 802.11 standards such as 802.11a, 802.11b, 802.11g, and 802.11n. 802.11b and 802.11g operate in the 2.4 GHz band, 802.11a operates in the 5 GHz band, and 802.11n can operate in both bands

Both WiFi and Bluetooth are based on spread spectrum signal structuring. With this radio transmission technique, a narrowband signal is expanded across a given portion of the radio frequency spectrum to result in a broader or wideband signal. Such a wideband signal provides a very strong immunity to interference compared to a narrowband signal.

Bluetooth uses Frequency Hopping Spread Spectrum (FHSS), whilst WiFi uses Direct Sequence Spread Spectrum (DSSS). Given that both technologies operate in the same frequency band, this use of differing techniques can result in interference issues. FHSS devices and DSSS devices perceive each other as noise.

Both Bluetooth and WiFi technologies, however, use sophisticated error detection and error correction techniques to deliver correct data. Additionally, if a transmission cannot be decoded due to interference, the transmission is resent. This interference will, of course, increase as the number of coexistent devices in proximity to each other increases. Due to the robust error detection mechanisms, however, as the interference level increases, data continues to be delivered correctly, but the data rate decreases as the number of dropped packets increases.

In terms of security, both systems use authentication with encryption and pin codes/pass words. In addition, the R40 itself uses a proprietary Interface Protocol thus preventing a non-authorized user from taking control of the device.

When transmitting wirelessly, data packages are time-stamped when acquired by the amplifier, before being transmitted, and when received by the application they are recorded according to this timestamp. In this way, there is no risk associated with delayed communications or missing data packets over a wireless link since, if the recording software detects missing packages, an event is inserted into the recording to notify the operator. In the extreme case whereby the interference causes the wireless link to be dropped all together, the application automatically reconnects when the interference is removed.



### Quality of Service and Associated Risks

1. The risk of corrupt data due to interference is very small due to error detection, error correction and resend data packet mechanisms. In addition to this error detection and correction, the application provides time-stamped data packages, which enables the detection of corrupt, delayed or missing data.
2. The risk of missing data due to interference is also very small, but at the extreme, the data rate decreases as more and more data packets have to be dropped and resent. Ultimately, in the presence of extreme interference, the data rate will decrease to zero and the wireless link will be dropped. This situation is also adequately handled with the provision of time-coded data packets, which enables the detection of corrupt, delayed or missing data. In the extreme case whereby the interference causes the wireless link to be dropped all together, the application automatically reconnects when the interference is removed. This situation is very similar to being out-of-range and the same mechanisms apply and, again, the application will automatically reconnect when the device comes back into range.

In the presence of extreme and persistent interference, the cabled USB connection is, of course, available.

3. The risk of unauthorised users is very small due to the authentication requirements of the wireless link and the fact that the R40 Interface Protocol is proprietary.
4. The medical system uses mature, industry-standard hardware and protocols: Bluetooth and WiFi. This ensures that the system utilises all the benefits associated with these mature standards, concerning the authentication, data integrity and interference performance as discussed in this document.
5. The radio modules are tested according to their own EMC emissions and immunity standards: EN 300 328, EN 301 489-1, EN 301 489-17 and IEC 60601-1-2 (Bluetooth).
6. The radio modules are pre-certified and Type Approved.

Considering the medical system function, its indication for use and very low risk associated with a low level of concern, the analysis, evaluation and preventative measures undertaken reveal the low risk associated with wireless communication. In the presence of extreme interference, the rate of delivery of data packets will decrease until ultimately, the wireless link is dropped. Wireless communication problems are identified, prevented and mitigated, as described. The application identifies these wireless problems and automatically reinstates the wireless link if dropped in the presence of extreme interference. Alternatively, the cabled USB connection is available.

### Pre-compliant Wireless Modules

The use of pre-compliant, certified and Type-approved optionally-fitted internal Bluetooth and WiFi wireless modules which comply with applicable national radio regulations ensures best performance, interoperability, coexistence and quality of service is achieved.

## Specifications (taken from Appendix 1).

### Bluetooth Module

#### Specifications:

- Type: Bluetooth 4.0.
- Output power: 11dBm max.
- Output frequency: 2.402 - 2.480 GHz, ISM band.
- Data rate: 1.3 Mbps max.
- Protocols: Standard Bluetooth - SPP, GATT, DUN, PAN.
- Modulation: GFSK, DQPSK. Frequency Hopping Spread-Spectrum (FHSS).
- Error Correction: Forward Error Correction (FEC), Automatic repeat request (ARQ).
- Security: authorization and authentication of devices, proprietary Interface Protocol.

#### Conformance:

- Type Approval: Europe (R&TTE), US (FCC/CFR 47 part 15), Canada (IC RSS).
- R&TTE Directive 1999/5/EC
- Effective use of frequency spectrum: EN 300 328
- EMC: EN 301 489-1, EN 301 489-17, EN 61000-6-2
- Health and safety: EN 62479, EN 60950-1, IEC 60950-1
- Medical Electrical Equipment IEC 60601-1-2
- Bluetooth Qualification v4.0.

### WiFi Module

#### Specifications:




- Type: 2.4 GHz IEEE Std. 802.11 b/g Wireless LAN Module
- Output power: 12dBm max.
- Output frequency: 2.412 to 2.462 GHz, ISM band.
- Data rate: 230kbps max.
- Protocols: TCP, UDP, DHCP, DNS, ICMP, ARP, HTTP Client, and FTP Client.
- Modulation: 802.11b Compatibility: DSSS (CCK-11, CCK-5.5, DQPSK-2, DBPSK-1) - 802.11g: OFDM.
- Error Correction: Forward Error Correction (FEC).
- Security: WEP-128, WPA-PSK (TKIP), WPA2-PSK (AES), proprietary Interface Protocol.

#### Conformance:

- Type Approval: Europe (R&TTE), US (FCC/CFR 47 part 15), Canada (IC RSS).
- R&TTE Directive 1999/5/EC
- Effective use of frequency spectrum: EN 300 328
- EMC: EN 301 489-1, EN 301 489-17
- Health and safety: EN 60950-1, EN50371

## Interference

The R40 Amplifier will continue to operate in the presence of radio frequency magnetic fields (RF) and the effects of electrostatic discharges (ESD) and other interference, in accordance with the requirements of IEC60601-1-2. However, the amplifier records signals of very low amplitude, and these signals themselves are not immune to the effects of RF, ESD and low-frequency magnetic field interference. Such interference may cause signal artefacts.

	Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Trackit R40, including cables specified by Lifelines Ltd. Otherwise, degradation of the performance of this equipment could result.
	When in close proximity to the amplifier, do not use mobile phones, transmitters, power transformers, motors, or other equipment that generates magnetic fields. Refer to the Appendix for more information.
	When using the amplifier in close proximity to other devices using Bluetooth or WiFi communication, orientate or position these devices for least interference. If possible separate the devices or turn off their wireless communication.

**NOTE:** Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in the Manufacturers Declaration in the Appendix.

## Appendix 4: Troubleshooting Guide

### COM port problems with Bluetooth communication to the R40

#### The COM port is available but is being used by another application.

This could well be the case if an application such as Microsoft Active Synch is installed and polling the COM port for a Windows CE device. Make sure Connection Mode for Active Synch is set to Only When Device is Connected, and not to Continuous.

Make sure other applications such as virus protection software and personal firewalls (ZoneAlarm) are not accessing the COM port while a connection to Trackit is being made.

### Problems starting the recording

#### The setup has not been sent correctly

Under R40 Status, in the Control Panel, check that Acquire Ready shows Yes. If it is not ready, acquisition cannot begin. This could be caused by incomplete transmission of the R40 setup.

Check that all channels in the Recording setup have the same sample rate. The R40 does not support multi-sample rate.

#### An incorrect setup has been sent

If an incompatible setup has been sent to the R40 the message; "unable to comply" will indicate that. If an incorrect setup has been sent, the Trackit Control Panel will show 'Acquire Ready: No'

#### The card is not formatted correctly

If the card is not formatted with a correct 32-bit FAT, a recording cannot commence. Format the flash card using the SD Card Formatter PC utility.

#### The card is corrupted

Disk corruption can be caused when a SD card is removed from the R40 or the Card reader while data is being written or accessed.

R40: always stop a recording and wait for the write LED to go out, before removing the card.

Card reader /PC: Always stop and eject the card using the icon in the Windows system tray before physically ejecting it.






#### The card is not inserted correctly

If the flash card is not pushed in far enough, the card will not engage the pins on the card reader. 'No disk present', in the Status section of the Trackit Control Panel, will confirm this.

## Appendix 5: Manufacturer's Declaration

### EMC Compatibility

This section contains specific information regarding the device's compliance with IEC 60601-1-2 and EN 60601-1-2.

	The use of accessories, transducers and cables other than those specified, with the exception of transducers and cables sold by the manufacturer of the equipment as replacement parts for internal components, may result in increased emissions or decreased immunity of the equipment.
	Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided here.
	The equipment or system should not be used adjacent to or stacked with other equipment and that if adjacent or stacked use is necessary, the equipment or system should be observed to verify normal operation in the configuration in which it will be used.
	Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the R40, including cables specified by Lifelines Ltd. Otherwise, degradation of the performance of this equipment could result.
	When in close proximity to the R40 Amplifier, do not use mobile phones, transmitters, power transformers, motors, or other equipment that generates magnetic fields.

Accessory name	Type	Length	Description
USB Interface Cable	USB	2.8 m	USB shielded cable
Input electrodes	EEG disc electrodes	1 m	Unshielded EEG disc electrodes
Input electrodes (E-cap)	EEG disc electrodes	1 m	Unshielded EEG disc electrodes
Nonin XPOD	Shielded	2 m	Nonin
Aux. Connector cable	Shielded	1 m	Shielded cable
Patient Event Switch	CM-5	2 m	Two-core unshielded cable

## Guidance and Manufacturer's Declaration

### Electromagnetic Emissions

#### IEC 60601-1-2 / EN 60601-1-2

The R40 is intended for use in the electromagnetic environment specified below. The customer or user of the R40 should assure that it is used in such an environment.


Emissions Test	Compliance	Electromagnetic Environment Guidance
RF emissions CISPR11/EN55011	Group 1	The R40 uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR11/EN55011	Class B	The R40 is suitable for use in all establishments, including domestic establishments and those directly connected to the public low voltage power supply network that supplies buildings used for domestic purposes. Note: Only the recommended or supplied PC must be used in the system to ensure compliance.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/Flicker emissions IEC 61000-3-3	Complies	

### Electromagnetic Immunity

#### IEC 60601-1-2 / EN 60601-1-2

The R40 is intended for use in the electromagnetic environment specified below. The customer or user of the R40 should assure that it is used in such an environment.

Immunity Test	EN 60601-1-2 Test Level	Compliance Level	Electromagnetic Environment Guidance
Electrostatic discharges (ESD) IEC 61000-4-2	+/- 8 kV: Contact +/- 15kV: Air	+/- 8 kV: Contact +/- 8kV :Air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.  While in use, the patient should be stationery and not touch the R40 amplifier
Electrical fast Transients/ burst IEC 61000-4-4	Compliance is provided by the recommended PC equipment.	Compliance is provided by the recommended PC equipment.	Mains power should be that of a typical commercial and/or hospital environment
Surge IEC 61000-4-5	Compliance is provided by the recommended PC equipment.	Compliance is provided by the recommended PC equipment.	Mains power should be that of a typical commercial and/or hospital environment
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	Compliance is provided by the recommended PC equipment.	Compliance is provided by the recommended PC equipment.	Mains power should be that of a typical commercial and/or hospital environment. If the user of the R40 system requires continued operation during power mains interruptions, it is recommended that the R40 system be powered from an uninterruptible power supply or a battery

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment Guidance
Power frequency (50/60Hz) magnetic field IEC 61000-4-8	3 A/m, 30A/m	3 A/m See Note e.	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial and/or hospital environment.
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz 6V in ISM Bands	3 Vrms	Portable and mobile RF communications equipment should be used no closer to any part of the R40, including cables than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.  <b>Recommended separation distance</b> $d = [3.5/E] \sqrt{P} = 1.2 \sqrt{P}$
Radiated RF Electromagnetic Fields IEC 61000-4-3	3 V/m 80 MHz to 2.5 GHz 10V/m (Home Environment)	3 V/m See Note f.	$d = [3.5/E] \sqrt{P} : 80 \text{ MHz to } 800 \text{ MHz} = 1.17 \sqrt{P}$ $d = [7/E] \sqrt{P} : 800 \text{ MHz to } 2.5 \text{ GHz} = 2.33 \sqrt{P}$  Note: using unshielded input leads  Where P is the maximum output power rating of the transmitter in watts (W) according to the manufacturer and d is the recommended separation distance in meters (m).  Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey <sup>a</sup> , should be less than the compliance level in each frequency range <sup>b</sup> .  Interference may occur in the vicinity of equipment marked with the following symbol: 
NOTE 1. At 80 MHz and 800 MHz, the higher frequency range applies.			
NOTE 2. These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			
a Field strength from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the R40 is used exceeds the applicable RF compliance level above, the R40 should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the R40.			
b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.			
c The immunity levels for conducted RF are for unshielded input electrode leads 1 m in length and worse-case coupling, including any resonances across the frequency band. The interference is less when the coupling plane of the interference source is not in the same plane as the electrode leads.			
d The immunity levels for radiated RF are for unshielded input electrode leads 1 m in length and worse-case coupling, including any resonances across the frequency band. The interference is less when the polarisation plane of the interference source is not in the same plane as the electrode leads.			
e The R40 does not contain magnetic components and is not susceptible to power frequency magnetic field interference.			
f The conditions of intended use justify lower immunity test levels. The hazards and risk analysis associated with these lower limits have been documented in the Risk Management file			

## Recommended separation distance between portable and mobile RF communications equipment and the R40 EEG System

### IEC 60601-1-2 / EN 60601-1-2

The R40 is intended for use in the electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the R40 can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the R40 as recommended below, according to the maximum output power of the communications equipment.

If any electromagnetic interference is encountered, the patient and equipment should move to an area without interference. In any case, the electromagnetic interference does not pose any risks to the patient, as the R40 is a non-invasive recording device that does not modify or interact with the patient.

Rated maximum output power of transmitter	Separation distance according to frequency of transmitter		
	150 kHz to 80 MHz $d = 1.17 \sqrt{P}$	80 MHz to 800 MHz $d = 1.17 \sqrt{P}$	800 MHz to 2.5 GHz $d = 2.33 \sqrt{P}$
W			
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

**NOTE:** At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

**NOTE:** These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.



# Version History

## V1.0 (4th March 2015)

- Initial release

## V1.1 (16th April 2015)

- Added "CAUTION: Federal (USA) law restricts this device to sale by or on the order of a physician" on page 8.
- Added "FDA cleared for use in USA" to EEG electrode warning on page 8.
- Added "The Amplifier is intended to be connected to a PC which is powered from a medically approved power supply" on page 8.
- Amended "Indications for Use" statement on page 8 and deleted "Intended Use".
- Added "Compliance is provided by the recommended PC equipment" to Electromagnetic Immunity tables in Appendix 5. Amended Bluetooth and WLAN specifications in Appendix 1.

## V1.2 (20th October 2015)

- Changed EN references to IEC.
- Amended sampling rate and bandwidth specifications.

## V1.3 (26th October 2015)

- Electromagnetic immunity compliance level amended on pages 39 & 40.

## V1.4 (27 February 2018)

- Added disinfection information in section 2.6.
- Added device lifetime in section 2.7.
- Change of N.B. to 0086 (BSI).

## V1.5 (20 August 2019)

- EMC warnings and information updated
- Additional cleaning wipes added for US customers.
- Trackit Software instructions updated

## V1.6 (14 October 2019)

- Notified Body change and EC Rep information added.
- Updated with new Cover page and images.

## V2.0 (5 March 2020)

- Updated with new design and images
- R40 (24) variant added.
- Trackit Software section moved to separate user manual



**Lifelines**  
neuro

# **R40** and **R40 24** EEG Amplifiers

**Lifelines Ltd,**

7 Clarendon Court, Over Wallop, near Stockbridge,

Hampshire SO20 8HU, UK

Telephone +44 (0)1264 782226

[www.LLines.com](http://www.LLines.com)

[sales@LLines.com](mailto:sales@LLines.com)

**Imagine EEG Anywhere**